





Insert the Hex Driver within the 30Ncm torque ratchet



Insert driver into abutment and turn torque ratchet clockwise until torque of 30 Ncm is reached and the head of the ratchet releases

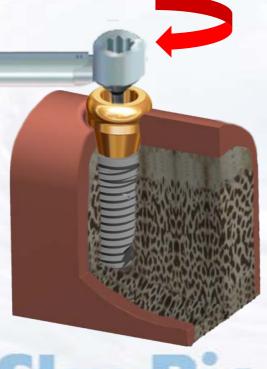


**Blue Sky Bio** 

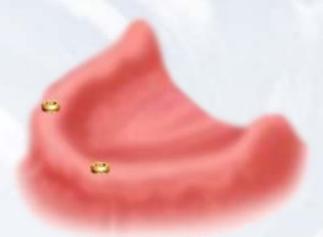


Abutments in place



Snap impression transfer on the abutments





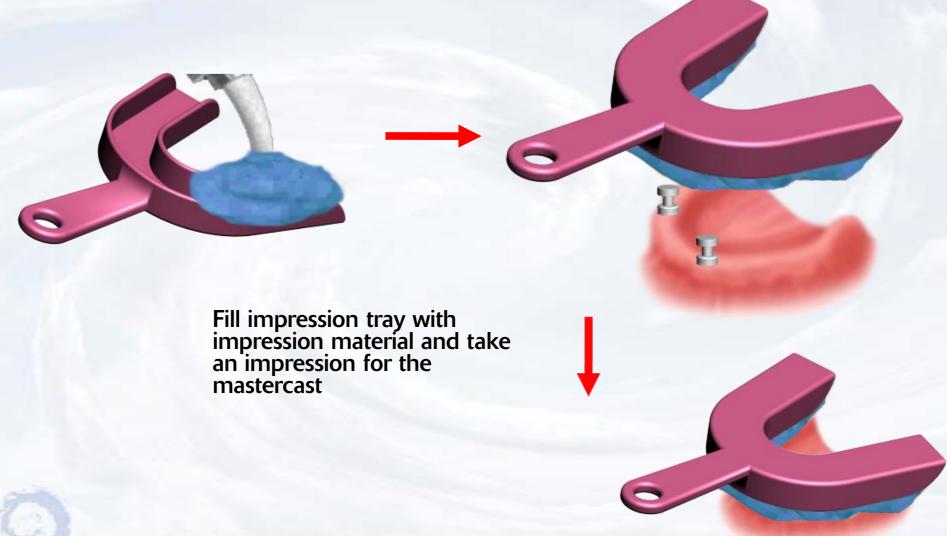




After impression material has set remove impression from mouth picking up the impression transfers


Snap analogs into the impression transfers



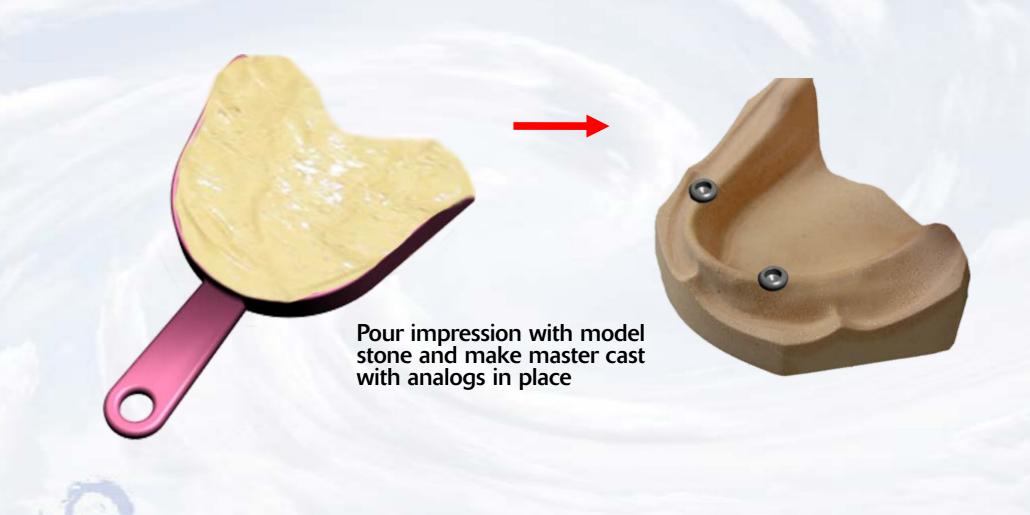











Remove the black processing insert with the sharp point of the removal instrument



Place the insert with the desired retention into the housing





Finished prosthesis with housings and inserts in place

